

Mouse /Rat IGF-I/IGF-1 ELISA Instructions

CAT. No: AEM0024

CONTENT

No.	Content	Cat. No	Volume
1	CP (Cotaed Plate)	EM0024 CP	96 wells
2	S (Standard)	EM0024S,S1~ S7,S0	9 vials
3	DA (Detect Antibody)	EM0024 DA	6 ml/bottle
4	SH(Streptavidin-HRP)	ESH01	12 ml/bottle
5	AB(Assay Buffer 1×)	EAB01	12 ml/bottle
6	SD (Sample Diluent)	ESD01	15 ml/bottle
7	TS (TMB Substrate)	ETS01	12 ml/bottle
8	SS (Stop Solution)	ESS01	12 ml/bottle
9	WB (Wash Buffer 10×)	EWB01	50 ml/bottle
10	SF (Sealer Film)	ESF01	6 pieces

NOTE: After the kit is opened, the stabilization period of each content is 30 days, so please use the kit within 30 days after opening.

SAMPLE DILUTION

Samples such as serum, plasma require at least a 400-fold dilution into Sample Diluent. A suggested 400-fold dilution is 10 µl of sample + 190 µl of Sample Diluent, after mixing, take out 10 µl intermediate concentration and add 190 µl Sample Diluent


REAGENT PREPARATION SAMPLE ample Dilution

Washing Buffer (1×) Preparation: Pour entire contents (50 ml) of the **Washing Buffer Concentrate** (10×) into a clean 500 ml graduated cylinder. Bring to final volume of 500 ml with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2 to 25°C.

Standard Curve Preparation: S1 to S7 and S0 is ready to use for serum and plasma.

Other sample type, prepare the standard curve with whatever buffer (SPB, Sample Prepared Buffer) is used to prepare the sample, such as cell culture supernatant, tissue grinding liquid, cell lysate, etc. Urine sample use AB (Assay Buffer) prepare standard curve.


The Mouse/Rat IGF-I/IGF-1 Standard EM0024S 50000 pg/ml 30 µl + 270 µl SPB serves as the high standard (5000 pg/ml). Pipette 200 µl of SPB into each tube. Use the high standard to produce a 1:2 dilution series. Mix each tube thoroughly before the next transfer. SPB serves as the zero standard (0 pg/ml).

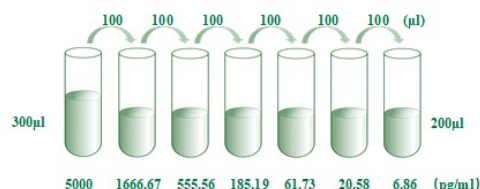

ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess **CP** (Coated Plate) strips from the plate frame, return them to the foil pouch and reseal.
3. Add 50 µl of **AB** (Assay Buffer) to each well.
4. Add 50 µl or 10 µl of **Standard or sample** per well. Ensure reagent addition is uninterrupted and completed within 15 minutes.
5. Add 50 µl of **DA** (Detect Antibody) to each well.
6. Cover with an **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 1 hour on a microplate **shaker** set at 500 rpm.
7. Aspirate each well and **wash**, repeating the process four times. Wash by filling each well with WB (Washing Buffer 300 µl). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining WB (Washing Buffer) by aspirating or decanting. Invert the plate and **blot** it against clean paper towels.
8. Add 100 µl of **SH** (Streptavidin-HRP) to each well.
9. Cover with a new **SF** (Sealer Film). Incubate at room temperature (18 to 25°C) for 30 minutes on a microplate **shaker** set at 500 rpm.
10. Repeat aspiration/**wash** as in step 7.
11. Add 100 µl of **TS** (TMB Substrate) to each well. Incubate for 5-30 minutes at room temperature.
12. Add 100 µl of **SS** (Stop Solution) to each well.
13. Determine the optical density within 30 minutes, using microplate **reader** set to 450 nm corrected with 570 nm or 630 nm.

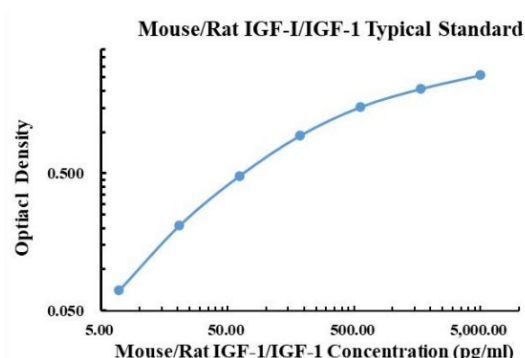

pg/ml	O.D.		Average	Corrected
0.00	0.0647	0.0635	0.0641	
6.86	0.1385	0.1303	0.1344	0.0703
20.58	0.2735	0.2724	0.2730	0.2089
61.73	0.5618	0.5279	0.5449	0.4808
185.19	1.0550	0.9549	1.0050	0.9409
555.56	1.6270	1.5390	1.5830	1.5189
1666.67	2.2390	2.0130	2.1260	2.0619
5000.00	2.6320	2.6820	2.6570	2.5930

SENSITIVITY

The minimum detectable dose (MDD) of Mouse/Rat IGF-I/IGF-1 is typically less than 1.76 pg/ml (50 µl of sample volume) or 3.43 pg/ml (10 µl of sample volume).

The MDD was determined by adding two standard deviations to the mean optical density value of ten zero standard replicates and calculating the corresponding concentration.

PRECISION

- Intra-assay Precision (Precision within an assay) Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.
- Inter-assay Precision (Precision between assays)

Sample Number	Intra-assay Precision			Sample Number	Inter-assay Precision		
	S1	S2	S3		S1	S2	S3
	22	22	22		6	6	6
Average (pg/ml)	119.3	509.0	1409.9		109.9	510.1	1498.1
Standard deviation	8.2	39.3	109.4		5.4	27.0	100.4
Coefficient of variation (%)	6.9	7.7	7.8		4.9	5.3	6.7

RECOVERY

The spike recovery was evaluated by spiking 3 levels of Mouse/Rat IGF-I/IGF-1 into health mouse serum sample. The un-spiked serum was used as blank in this experiment.

The recovery ranged from 94% to 105% with an overall mean recovery of 101%.

LINEARITY

To assess the linearity of the assay, five samples were spiked with high concentration of IGF-1/IGF-1 in Mouse/Rat serum and diluted with Sample Diluent to produce samples with values within the dynamic range of the assay.

The linearity ranged from 97% to 102% with an overall mean recovery of 100%.

SAMPLE VALUES

Serum/Plasma - Thirty samples from apparently healthy mice were evaluated for the presence of Mouse/Rat IGF-I in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (ng/ml)	Detectable %	Mean of Detectable (ng/ml)
Serum	30	4.93-460.32	100	135.06

Serum/Plasma - Thirty samples from apparently healthy rats were evaluated for the presence of Mouse/Rat IGF-I in this assay. No medical histories were available for the donors.

Sample Matrix	Sample Evaluated	Range (ng/ml)	Detectable %	Mean of Detectable (ng/ml)
Serum	30	84.54-1888.06	100	584.19

n.d. = non-detectable. Samples measured below the sensitivity are considered to be non-detectable.

DISCLAIMER AND VERSION

For research use only. Not for use in clinical diagnostic procedures.

Copyright 2024 AREX Biosciences Ltd. Version.240820